


USER ACTIVITIES: ARMY - CE
NAVY - MC

W-57-09

FED. SUP. CLASS
6630

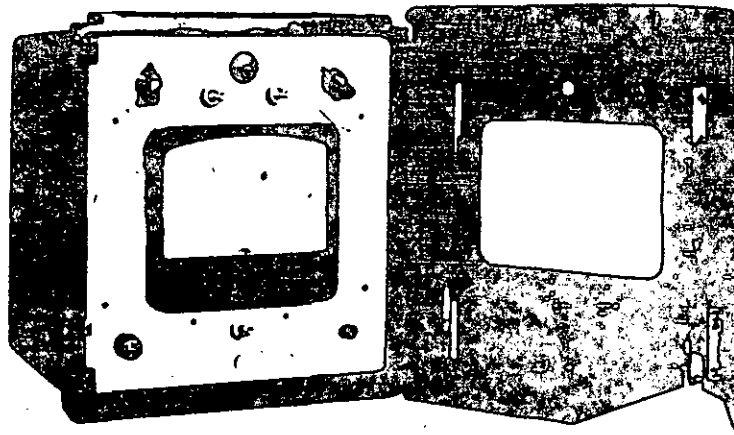

PART
NUMBER

PH

CANCELLED

CANCELLED AFTER 28 JAN 1982 NO SUPER-
SEDING STANDARD

The case shall be moisture and splash-proof. The face of the chassis with the dial gage shall be mounted on tracks inside the case to facilitate cleaning and maintenance. Meter shall have the following limits: 0.07 pH unit, 5 mv on the 700 mv range, and 10 mv on the 100 mv range. Scale shall be graduated in 0.1 pH, 5 mv, and 10 mv divisions.

Use: To continuously monitor a flow system for pH or oxidation-reduction potentials.

NOTE:

Items differing from this Military Standard by minor variations in design or dimensions are considered standard under this document provided such variations do not affect performance and are not in conflict with the material requirements as specified herein.



CANCELLED

U. S. GOVERNMENT PRINTING OFFICE: 1964-341-512/A-2125

P.A.	HU	TITLE	MILITARY STANDARD
Other Cust	MS 82	METER, HYDROGEN ION TEST Panel	MS36468
Procurement Specification	NONE	SUPERSEDES:	SHEET 1 OF 1

DD FORM 672 (Coordinated)

THIS DOCUMENT IS NOT TO BE USED

APPROVED 70268
REVISED 28 JAN 1982

This military standard is approved by the DoD for use by all activities. Selection for all applications and for repetitive use shall be as follows: